

# Human IGFBP – 3 total ELISA

## (Human Insulin-like Growth Factor Binding Protein-3)

Cat. No.: RMEE03A



European Union: for in vitro diagnostic use

Rest of the world: for research use only!

### INSTRUCTION FOR USE

IGFBP-3 ELISA	96 Determinations
CE	DE/CA40/00809/22
Principle of the test	Sandwich ELISA
Duration (incubation period)	2.5 h
Antibody-HRP-Conjugate	ready for use
Buffer and Substrate	ready for use
Standards	5 single standards: 0.4 - 30 ng/mL, lyophilized, human IGFBP-3
Assay Range	0.03 – 15150 ng/mL
Control	2 control sera, lyophilised
Sample	human serum / plasma
Required sample volume	10 µL
Sample dilution	1:505
Analytical sensitivity	0.03 ng/mL
average Intra- / Inter-Assay Variance	1.9% / 5.7%
Reference Values	Blum W.F et.al.1990 Insulin-Like Growth Factors and Their Binding Proteins. In: Ranke MB, Mullins P.E.(ed): Diagnostics of Endocrine Function in Children and Adolescents. Basel, Karger, 2011, pp.157-181

## INTENDED USE

This enzyme immunoassay kit is suited for measuring IGFBP-3 in human serum, EDTA and Heparin-plasma for diagnostic and scientific purposes.

## INTRODUCTION

Insulin-like growth factors (IGF)-I and -II are bound to specific binding proteins (IGFBPs) in the circulation. To date, at least six binding proteins can be distinguished on the basis of their amino acid sequence. They are designated as IGFBP-1, IGFBP-2, ... IGFBP-6 (1). The predominating IGFBP in blood is IGFBP-3, which largely determines the total IGF-I and IGF-II concentration. In contrast to the other binding proteins, IGFBP-3 has the property to associate with an acid-labile subunit (ALS) after binding of either IGF-I or IGF-II (3-5). Most of the IGFBP-3 in plasma is present as high molecular weight ternary complex, however, small amounts of free IGFBP-3 are also found (6,7).

The development of a specific immunoassays for IGFBP-3, which detects IGFBP-3 in the ternary complex, provided new in-sights into IGFBP-3 regulation (6-9). On the basis of these findings serum IGFBP-3 has been proven to be an additional useful test in the repertoire of diagnostic tools for evaluation of growth disorders (7,8).

Several factors besides GH influence IGFBP-3 levels: age including sexual development, nutrition, hypothyroidism, diabetes mellitus, liver function and kidney function. IGFBP-3 levels are decreased by malnutrition, although less than IGF-I, in hypothyroidism, in diabetes mellitus and in hepatic failure (6-8), but are increased in chronic renal failure (6,10,11). Measurement over 24 hours revealed no circadian rhythm (12,13). For clinical practice, the most important regulatory factor is GH. Single IGFBP-3 measurements correlate significantly with the logarithm of the integrated spontaneous GH secretion (8,14). In patients with GH deficiency, IGFBP-3 levels are subnormal and increase gradually to within the normal range after several days of GH administration (7,8). The slow response to GH and constant circadian levels during chronic daily application of GH (13) suggest that IGFBP-3 reflects the GH secretory state over days.

The major advantages of IGFBP-3 over IGF-I are:

1. No extraction step is required prior to measurement thus improving test accuracy by simplifying the assay procedure.
2. The normal range in young children is comparatively high making the detection of subnormal levels more reliable.
3. Patients with GH deficiency have subnormal IGFBP-3 levels. In contrast, most of the small statured children with normal GH secretion have levels within the normal range (Figure 1). The separation of these two groups is easy. In small statured children IGFBP-3 levels rise to normal range within several days of GH administration and remain normal during continuous GH treatment (Figure 2). Therefore, serum IGFBP-3 measurements are also suited for evaluating the potential of a patient to respond to GH and for GH therapy monitoring (19). In other patients of severe short stature, e.g. Ullrich-Turner syndrome or Silver-Russell syndrome, IGFBP-3 levels were found normal

(8) reflecting normal GH secretion.

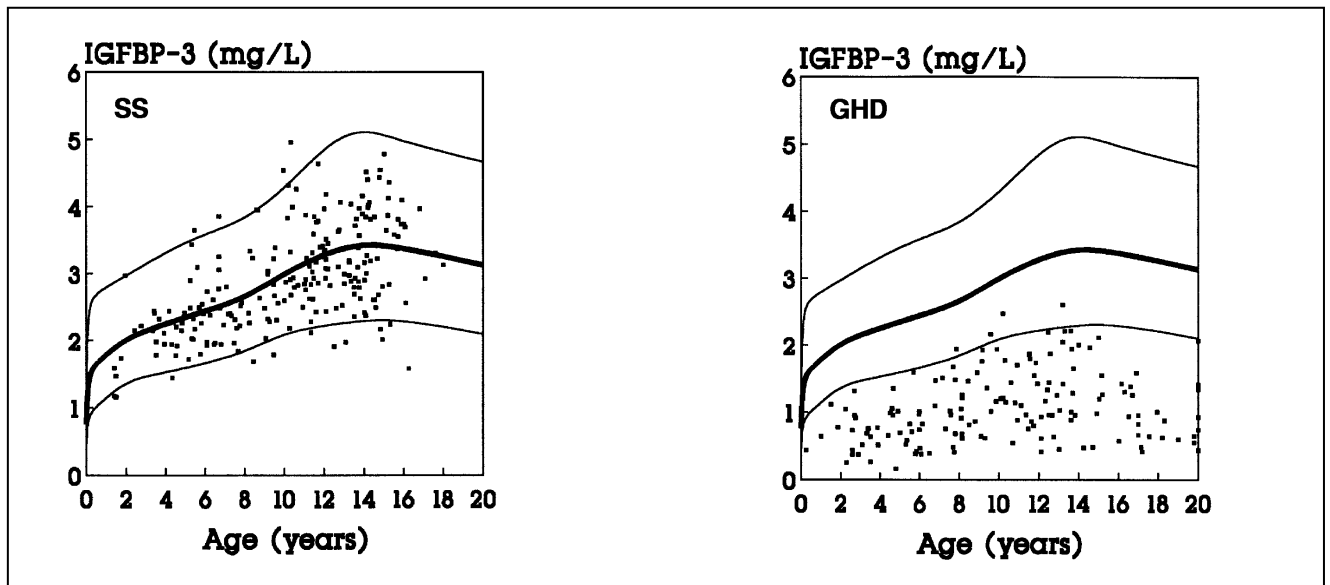


Fig. 1: Serum IGFBP-3 levels in patients with short stature without GH deficiency (SS: constitutional delay of growth and adolescence, familial short stature, intra-uterine growth retardation) and in idiopathic or organic GH deficiency (GHD). The normal range is given by the 5th, 50th and 95th percentile.


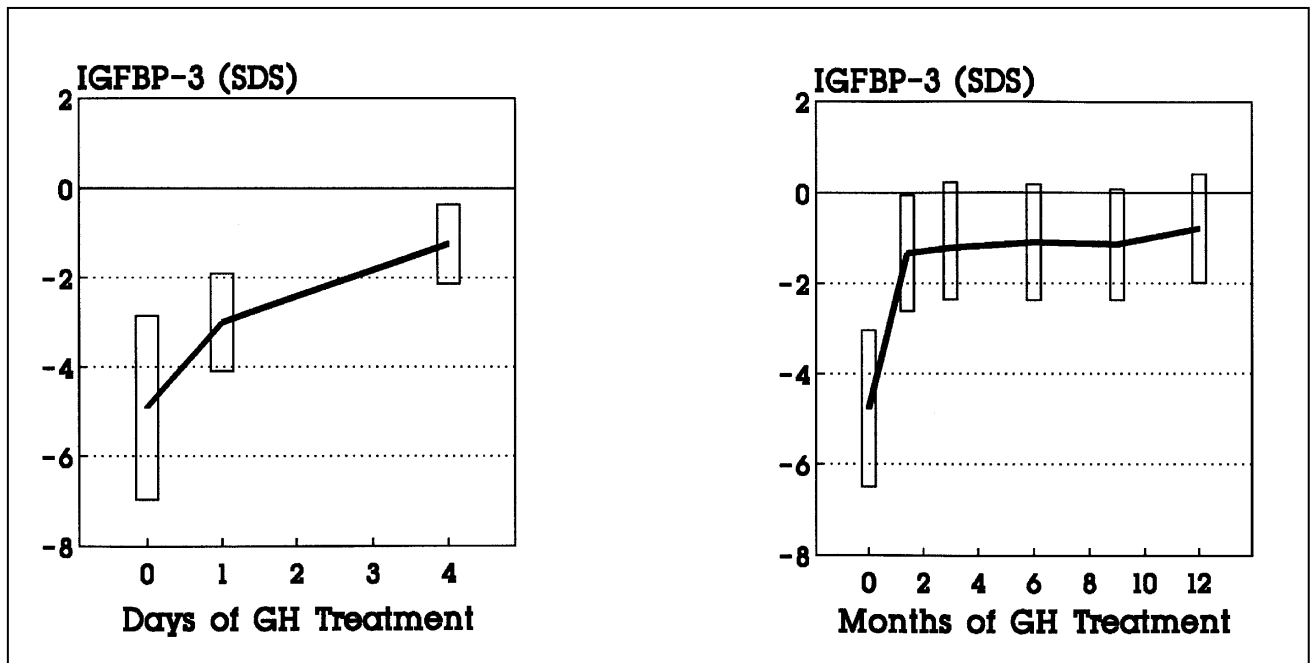


Fig. 2: IGFBP-3 levels in GH deficient children before and during GH treatment. Because of the age-dependence, values are given as the mean of standard deviation scores (SDS).

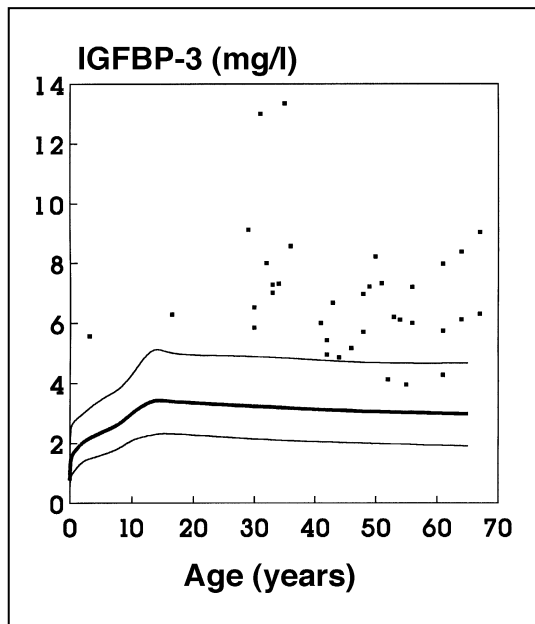

In normal tall children and adolescents without excessive GH secretion or in patients with Sotos syndrome, IGFBP-3 levels are normal or slightly increased. In contrast, children with pituitary gigantism or adults with acromegaly have clearly elevated levels (Figure 3) (6,15) that normalize on successful treatment. Therefore, IGFBP-3 is also a useful parameter for the detection of excessive GH secretion and monitoring therapy efficacy. In precocious puberty, IGFBP-3 levels are clearly increased by chronological age, whereas patients with premature thelarche have IGFBP-3 levels in the upper normal range (15).

Fig. 3: Serum IGFBP-3 levels in acromegaly. The normal range is given by the 5th, 50th and 95th percentile.

## ASSAY PRINCIPLE

The Mediagnost ELISA for IGFBP-3 E03A is a so-called Sandwich-Assay. It utilizes two specific antibodies of high affinity. First the IGFBP-3 in the sample binds to the immobilized antibody on the microtiter plate. In the following step, the complex of biotinylated anti-IGFBP-3-Antibody and Streptavidin-Peroxidase binds in turn to the immobilised IGFBP-3. Subsequently, the peroxidase catalyzes an enzymatic reaction resulting in a blue coloration. The intensity of the blue color depends on the IGFBP-3 content of the sample. The reaction is stopped by the addition of stop solution and color intensity is quantified by measuring the absorption.

## WARNINGS AND PRECAUTIONS

**For In Vitro Diagnostic Use only. For Professional use only.**

The Mediagnost kit is suitable only for in vitro diagnostics and not for internal use in humans and animals. Follow strictly the test protocol. Use the valid version of the package insert provided with the kit. Be sure that everything has been understood. Mediagnost will not be held responsible for any loss or damage (except as required by statute) howsoever caused, arising out of noncompliance with the instructions provided.

Do not use obvious damaged or microbial contaminated or spilled material.

**Caution: This kit contains material of human and/or animal origin. Therefore all components and patient's specimens should be treated as potentially infectious.**

Appropriate precautions and good laboratory practices must be used in the storage, handling and disposal of the kit reagents. The disposal of the kit components must be made according to the local regulations.

### Human Serum

Following components contain human serum: **Control Sera KS1 / KS2, Standards A-E**

Source human serum for the control sera provided in this kit was tested and found non-reactive for Hepatitis-B surface antigen (HBsAg), Hepatitis C virus (HCV), and Human Immunodeficiency Virus 1 and 2 (HIV). No known methods can offer total security of the absence of infectious agents; therefore all components and patient's specimens should be treated as potentially infectious.

### Reagents AK, VP, WP

Contain as preservative **5-chloro-2-methyl-4-isothiazolin-3-one and 2-methyl-4-isothiazolin-3-one** (<0.015%)

H317	May cause an allergic skin reaction.
P280	Wear protective gloves/ protective clothing/ eye protection/ face protection.
P272	Contaminated work clothing should not be allowed out of the workplace.
P261	Avoid breathing dust/ fume/ gas/ mist/ vapours/ spray.
P333+P313	If skin irritation or rash occurs: Get medical advice/ attention.
P302+P352	IF ON SKIN: Wash with plenty of soap and water.
P501	Dispose of contents/ container in accordance with local/ regional/ national/ international regulations.

### Substrate Solution (S)

The TMB-Substrate (S) contains 3,3',5,5' Tetramethylbenzidine (<0.05%)

H315	Causes skin irritation.
H319	Causes serious eye irritation.
H335	May cause respiratory irritation.
P261	Avoid breathing dust/ fume/ gas/ mist/ vapours/ spray.
P305+P351+	IF IN EYES: Rinse cautiously with water for several minutes.
P338	Remove contact lenses, if present and easy to do. Continue rinsing.

### Stopping Solution (SL)

The Stopping solution contains 0.2 M acid sulphuric acid (H<sub>2</sub>SO<sub>4</sub>)

H290	May be corrosive to metals.
H314	Causes severe skin burns and eye damage.
P280	Wear protective gloves/ protective clothing/ eye protection/ face protection.

P301+P330+	IF SWALLOWED: rinse mouth.
P331	Do NOT induce vomiting.
P305+P351+	IF IN EYES: Rinse cautiously with water for several minutes.
P338	Remove contact lenses, if present and easy to do. Continue rinsing.
P309+P310	IF exposed or if you feel unwell: Immediately call a POISON CENTER or doctor/physician.

#### **General first aid procedures:**

Skin contact: Wash affected area rinse immediately with plenty of water at least 15 minutes. Remove contaminated cloths and shoes.

Eye contact: In case of contact with eyes, rinse immediately with plenty of water at least 15 minutes. In order to assure an effectual rinsing spread the eyelids.

Ingestion: After swallowing the product, if the affected person is conscious, rinse out the mouth with plenty of water: seek medical advice immediately.

## **SAMPLES**

#### **Samples type**

Serum and Plasma

Serum and Heparin/EDTA Plasma yield comparable values.

#### **Speciment collection**

Use standard venipuncture for the blood sampling. Haemolytic reactions have to be avoided.

**Required sample volume: 10 µL**

#### **Sample stability**

In firmly closable sample vials

- Storage at 20-25°C: 3 days
- Storage at -20° C: min. 2 years
- Freeze-thaw cycles max. 10

The storage of samples over a period of 2 years at -20°C, showed no influence on the reading. Freezing and thawing of samples should be minimized. 10 Freezing-Thawing showed no effect on samples.

#### **Interference**

Triglyceride, bilirubin and hemoglobin in the sample do not interfere to a concentration of 100 mg/mL, 100 µg/mL or 5 mg/mL, respectively. However, the use of haemolytic, lipemic or icteric samples should be validated by the user.


### Sample dilution

- Dilution: **1:505** with Sample Buffer **PP**
- Pipette **1 ml Sample Buffer PP** (red colored) in PE-/PP-Tubes (application of a multi-stepper is recommended in larger series), add **10 µL Serum- or Plasma** (dilution factor 101). Add **400 µL Sample Buffer PP** in another PE-/PP-tube and **100 µL** of the thoroughly mixed first dilution (dilution factor 5). After mixing use **50 µL** of this 1:505 diluted solution **within 1 hour per determination** in the assay.
- Sample stability after dilution of the sample: maximum 1 hour at 20-25°C.

## MATERIALS

### Materials provided

The reagents listed below are sufficient for 96 wells including the standard curve.

<b>MTP</b>	<b>Microtiter plate</b> , ready for use, coated with rabbit-anti-hIGFBP-3-antibody. Wells are separately breakable.	<b>(8x12) wells</b>
<b>A-E</b>	<b>Standards</b> , lyophilized, (human IGFBP-3), concentrations are given on vial labels and on the QC-certificate.	<b>5 x 1 mL</b>
<b>KS1</b>	<b>Control Serum 1</b> , lyophilised, (human serum), concentration is given on the QC-certificate.	<b>1 x 250 µL</b>
<b>KS2</b>	<b>Control Serum 2</b> , lyophilised, (human serum), concentration is given on the QC-certificate.	<b>1 x 250 µL</b>
<b>AK</b>	<b>Antibody-HRP-Conjugate</b> , ready for use, contains rabbit biotinylated anti-hIGFBP-3 antibody.	<b>1 x 12 mL</b>
<b>PP</b>	<b>Sample Buffer</b> , red color, ready for use, <b>Please shake before use!</b>	<b>1 x 120 mL</b>
<b>VP</b>	<b>Dilution Buffer</b> , ready for use, <b>Please shake before use!</b>	<b>1x 30 mL</b>
<b>WP</b>	<b>Washing Buffer</b> , 20-fold concentrated solution	<b>1 x 50 mL</b>
<b>S</b>	<b>Substrate</b> , ready for use, horseradish-peroxidase-(HRP) substrate, stabilised H <sub>2</sub> O <sub>2</sub> Tetramethylbencidine.	<b>1 x 12 mL</b>
<b>SL</b>	<b>Stopping Solution</b> , ready for use, 0.2 M sulphuric acid.	<b>1 x 12 mL</b>
-	<b>Sealing Tape</b> , for covering the <b>microtiter plate</b> .	<b>2 x</b>
	<b>Instructions for use</b>	<b>1 x</b>
--	<b>Quality Control Certificate</b>	<b>1 x</b>

### Materials required, but not provided

- Distilled (Aqua destillata) or deionized water for dilution of the Washing Buffer WP (A. dest.), 950 mL.
- Precision pipettes and multichannel pipettes with disposable plastic tips
- Polyethylene PE/Polypropylene PP tubes for dilution of samples
- Vortex-mixer
- Microtiter plate shaker (350 rpm)
- Microtiter plate washer (recommended)
- Micro plate reader ("ELISA-Reader") with filter for 450 and  $\geq 590$  nm

## TECHNICAL NOTES

### Storage Conditions

Store the kit at 2-8°C after receipt until its expiry date. The lyophilized reagents should be stored at -20 °C after reconstitution. Avoid repeated thawing and freezing.

### Storage Life

The shelf life of the components **after initial opening** is warranted for **4 weeks**, store the unused strips and microtiter wells **airtight** together with the desiccant at 2-8°C in the clip-lock bag, use in the frame provided. The **reconstituted components** standards **A-E** and Control Sera **KS1** and **KS2** must be stored at -20°C (max. 4 weeks). For further use, thaw quickly but gently (avoid temperature increase above room temperature and avoid excessive vortexing). Up to 3 of the freeze-thaw cycles did not influence the assay. The 1:20 diluted Washing Buffer **WP** is 4 weeks stable at 2-8°C

### Preparation of reagents

Bring all reagents to room temperature (20 - 25°C) before use. Possible precipitations in the buffers have to be resolved before usage by mixing and / or warming. Reagents with different lot numbers cannot be mixed.

### Reconstitution

The Standards **A – E** and Controls **KS1 and KS2** are reconstituted with the Sample Buffer **PP**. It is recommended to keep reconstituted reagents at room temperature for 15 minutes and then to mix them thoroughly but gently (no foam should result) with a Vortex mixer.

### Dilution

After reconstitution dilute the Control Sera **KS1 and KS2** with the Sample Buffer **PP** in the same ratio (1:505) as the sample.

The required volume of Washing Buffer **WP** is prepared by 1:20 dilution of the provided 20fold concentrate with Aqua dest.



## Assay Procedure

When performing the assay, Blank, Standards **A-E**, Control Serum **KS1 and KS2** and the samples should be pipette as fast as possible (e.g. <15 minutes). To avoid distortions due to differences in incubation times, Antibody-HRP-Conjugate **AK** as well as the succeeding Substrate Solution **S** should be added to the plate in the same order and in the same time interval as the samples. Stopping Solution **SL** should be added to the plate in the same order as Substrate Solution **S**.

All determinations (Blank, Standards **A-E**, Control Sera **KS1 and KS2** and samples) should be assayed in duplicate. For optimal results, accurate pipetting and adherence to the protocol are recommended.

## Incubation

**Incubation at room temperature means: Incubation at 20 - 25°C.** The Substrate Solution **S**, stabilised H<sub>2</sub>O<sub>2</sub>-Tetramethylbendidine, is photosensitive—store and incubation in the dark.

## Shaking

The incubation steps should be performed at mean rotation frequency of a particularly suitable microtiter plate shaker. We are recommending 350 rpm. Due to certain technical differences deviations may occur, in case the rotation frequency must be adjusted. Insufficient shaking may lead to inadequate mixing of the solutions and thereby to low optical densities, high variations and/ or false values, excessive shaking may result in high optical densities and/ or false values.

## Washing

Proper washing is of basic **importance** for a secure, reliable and precise performance of the test. Incomplete washing is common and will adversely affect the test outcome. Possible consequences may be uncontrolled unspecific variations of measured optical densities, potentially leading to false results calculations of the examined samples. Effects like high background values or high variations may indicate washing problems.

All washing must be performed with the provided Washing Buffer **WP** diluted to usage concentration. Washing volume per washing cycle and well must be 300 µL at least.

The danger of handling with potentially infectious material must be taken into account.

When using an **automatic microtiter** plate washer, the respective instructions for use must be carefully followed. Device adjustments, e.g. for plate geometry and the provided washing parameters, must be performed. Dispensing and aspirating manifold must not scratch the inside well surface. Provisions must be made that the remaining fluid volume of every aspiration step is minimized. Following the last aspiration step of each washing cycle, this could be controlled, and possible remaining fluid could then be removed, by inverting the plate and repeatedly tapping it dry on non-fuzzy absorbent tissue.

**Manual washing** is an adequate alternative option. Washing Buffer may be dispensed via a multistepper device, a multichannel pipette, or a squirt bottle. The fluid may be removed by dynamical swinging out the microtiter plate over a basin. If aspirating devices are used, care has to be taken that the inside well surface is not scratched. Subsequent to every single washing step, the remaining fluid should be removed by inverting the plate and

repeatedly tapping it dry on non-fuzzy absorbent tissue.

### ASSAY PROCEDURE

Preparation of reagents		Reconstitution:	Dilution
A-E	Standards	in 1 mL Sample Buffer PP	-
KS1	Control Serum 1	in 250 µL Sample Buffer PP	1:505 with PP
KS2	Control Serum 2	in 250 µL Sample Buffer PP	1:505 with PP
WP	Washing Buffer	-	1:20 with Aqua dest.
<b>Sample dilution: with Sample Buffer PP 1:505</b>			
Before assay procedure bring all reagents to room temperature <b>20-25°C</b> .			
Assay Procedure in Double Determination:			
Pipette	Reagents	Position	
50 µL	Dilution Buffer VP	Pipette in <u>all</u> required number of wells	
50 µL	Sample Buffer PP as Blank	A1/A2	
50 µL	Standard A (0.4 ng/mL)	B1/B2	
50 µL	Standard B (2 ng/mL)	C1/C2	
50 µL	Standard C (6 ng/mL)	D1/D2	
50 µL	Standard D (15 ng/mL)	E1/E2	
50 µL	Standard E (30 ng/mL)	F1/F2	
50 µL	Control Serum KS 1 (1:505 diluted)	G1/G2	
50 µL	Control Serum KS 2 (1:505 diluted)	H1/G2	
50 µL	Sample (1:505 diluted)	in the rest of the wells according the requirements	
Cover the wells with the sealing tape.			
<b>Sample Incubation: 1 h at 20-25°C, 350 rpm</b>			
5 x 300 µL	Aspirate the contents of the wells and <b>wash</b> 5 x with 300 µL each Washing Buffer WP/ <b>well</b>	In each well	
100 µL	Antibody-POD-Conjugate AK	In each well	
Cover the wells with the sealing tape.			
<b>Incubation: 1 hour at 20-25°C, 350 rpm</b>			
5 x 300 µL	Aspirate the contents of the wells and <b>wash</b> 5 x with 300 µL each Washing Buffer WP/ <b>well</b>	In each well	
100 µL	Substrate Solution S	In each well	
<b>Incubation: 30 Minutes in the Dark at 20-25°C</b>			
100 µL	Stopping Solution SL	In each well	

	Measure the absorbance within 30 min at <b>450 nm</b> with $\geq 590$ nm as reference wavelength.	
--	---	--

## QUALITY CONTROL

Good laboratory practice requires that controls are included in each assay. A statistically significant number of controls should be assayed to establish mean values and acceptable ranges to assure proper performance. The test results are only valid if the test has been performed following the instructions. Moreover the user must strictly adhere to the rules of GLP (Good Laboratory Practice) or other applicable federal, state or local standards/laws. All standards and kit controls must be found within the acceptable ranges as stated on the QC Certificate. If the criteria are not met, the run is not valid and should be repeated. Each laboratory should use known samples as further controls.

### Quality criteria

For the evaluation of the assay it is required that the absorbance values of the blank should be below 0.25, and the absorbance of standard E should be above 1.00.

Samples, which yield higher absorbance values than Standard E, should be re-tested with a higher dilution.

## EVALUATION OF RESULTS

### Establishing of the standard curve

The standards provided contain the following concentrations of hIGFBP-3

Standard	A	B	C	D	E
ng/mL	0.4	2	6	15	30

- 1) Calculate the **mean absorbance** value for the blank from the duplicated determination (well A1/A2).
- 2) Subtract the mean absorbance of the blank from the mean absorbances of all other samples and standards.
- 3) Plot the standard concentrations on the x-axis versus the mean value of the absorbance of the standards on the y-axis.
- 4) Recommendation: Calculation of the standard curve should be done by using a computer program, because the curve is in general (without respective transformation) not ideally described by linear regression. **A higher-grade polynomial, or four parametric logistic (4-PL) curve fit or non-linear regression** are usually suitable for the evaluation (as might be spline or point-to-point alignment in individual cases).
- 5) The IGFBP-3 concentration in ng/mL (or pg/mL, according the chosen unit for the standards) of the samples can be calculated by **multiplication** with the respective **dilution factor**.

### Example of a typical standard curve

The following data is for demonstration only and cannot be used in place of data generation at the time of assay.

	Blank	A	B	C	D	E
ng/mL	0.0	0.4	2	6	15	30
OD <sub>(450-620 nm)</sub>	0.204	0.254	0.453	0.911	1.706	2.390

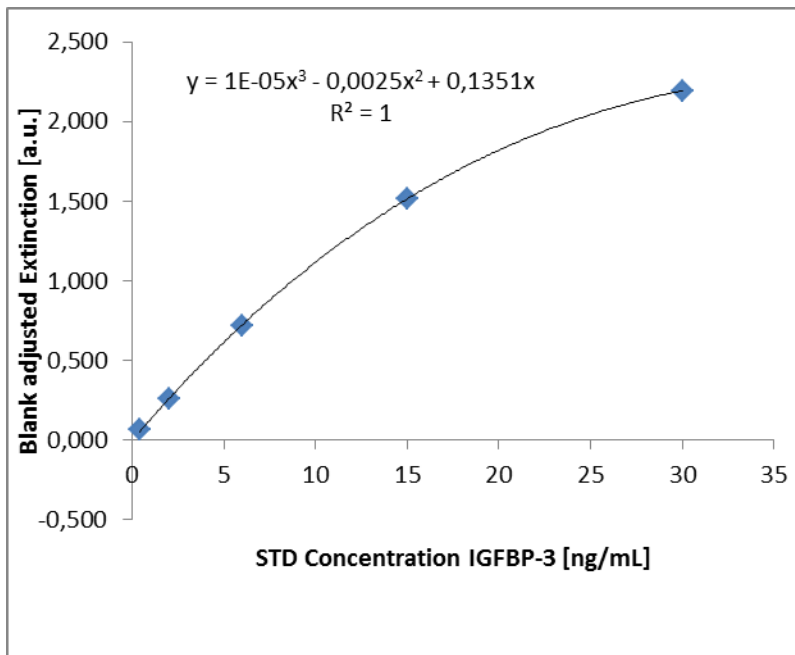


Fig. 4: Exemplary standard curve

The exemplary shown standard curve in Figure 4 **cannot** be used for calculation of your test results. You have to establish a standard curve for each test you conduct!

#### Exemplary calculation of IGFBP-3 concentrations

Sample dilution: 1:505

Measured extinction of your sample 0.975

Measured extinction of the blank 0.204

Your measurement program will calculate the IGFBP-3 concentration of the diluted sample automatically by using the difference of sample and blank for the calculation. You only have to determine the most suitable curve fit (here: polynomial  $x^{\text{rd}}$  degree).

In this exemplary case the following equation is solved by the program to calculate the IGFBP-3 concentration in the sample:

$$0.771 = 1E-05x^3 - 0.0025x^2 + 0.1351x$$

$$6.617 = x$$

If the dilution factor (**1:505**) is taken into account the IGFBP-3 concentration of the undiluted sample is

$$6.617 \text{ ng/mL} \cdot 505 = 3342 \text{ ng/mL} = 3,342 \text{ mg/L}$$

### **Interpretation of results**

The test results should not be the only base for therapeutic decisions. The results should be interpreted in regard to anamnesis, further clinical observations and results of other diagnostic investigations. Further, it is recommended to establish reference and cut-off values corresponding to the relevant group of patients for each laboratory.

### **LIMITATION OF PROCEDURE**

IGFBP-3 levels are strongly dependent on GH secretion. However, a number of factors influence its plasma concentration and should be taken into account for appropriate interpretation. Plasma levels decrease during fasting (more than 1 day), in malnutrition, malabsorption, cachexia, impaired hepatic function, hypothyroidism, and diabetes mellitus. They may also be decreased in chronic inflammatory disease and malignancy. Levels are increased in states of impaired renal function and precocious puberty. In clinical situations with hyperprolactinemia or in patients with craniopharyngeoma, normal levels may be observed despite GH deficiency.

In certain physiological (e.g. pregnancy) and pathological states, IGFBP-3 may be degraded to smaller molecular size compounds (16,17) by specific proteases which affect IGFBP patterns seen in Western ligand blotting, but in general only have little influence on the outcome of ELISA determinations. In case of special interest in this physiological process, the Mediagnost ELISA for **functional IGFBP-3 E04A** is available. The ELISA E04A enables to quantify the degree of IGFBP-3 fragmentation in samples.

The Mediagnost IGFBP-3 ELISA, E03A is based on polyclonal rabbit antibodies. Generally, this technique is sensible to heterophilic antibodies in the sample. The influence of heterophilic antibodies is reduced by assay design, but cannot be excluded completely.

### **REFERENCE VALUES**

IGFBP-3-levels are strongly age-dependent in children, less so in adults. The normal ranges in various age-groups which were log-normally distributed are given in table 1 by the percentiles (see Appendix). A graphic presentation is shown in Figure 5 and 6. It is recommended for each laboratory to establish its own normal range.

**Tab. 1:** Serum levels of IGFBP-3 in healthy subjects at various ages. Individuals between 7 and 17 years of age were classified according to gender, as the pubertal peak occurs almost 2 years earlier in girls than in boys.

Age group	Percentiles													
	0.1	1	5	10	20	30	40	50	60	70	80	90	95	99
0-1 week	<b>0.25</b>	0.33	<b>0.42</b>	0.48	<b>0.57</b>	0.64	<b>0.70</b>	0.77	<b>0.85</b>	0.93	<b>1.05</b>	1.23	<b>1.41</b>	1.81
1-4 weeks	<b>0.49</b>	0.62	<b>0.77</b>	0.86	<b>0.99</b>	1.10	<b>1.19</b>	1.29	<b>1.40</b>	1.52	<b>1.68</b>	1.93	<b>2.16</b>	2.68
1-3 months	<b>0.55</b>	0.70	<b>0.87</b>	0.98	<b>1.13</b>	1.25	<b>1.36</b>	1.48	<b>1.61</b>	1.75	<b>1.94</b>	2.23	<b>2.52</b>	3.14
3-6 months	<b>0.64</b>	0.80	<b>0.98</b>	1.10	<b>1.25</b>	1.38	<b>1.49</b>	1.61	<b>1.74</b>	1.88	<b>2.07</b>	2.37	<b>2.65</b>	3.24
6-12 months	<b>0.71</b>	0.88	<b>1.07</b>	1.19	<b>1.35</b>	1.48	<b>1.60</b>	1.72	<b>1.85</b>	2.00	<b>2.19</b>	2.49	<b>2.76</b>	3.36
1-3 years	<b>1.02</b>	1.21	<b>1.41</b>	1.53	<b>1.69</b>	1.82	<b>1.94</b>	2.05	<b>2.17</b>	2.31	<b>2.48</b>	2.74	<b>2.98</b>	3.47
3-5 years	<b>1.08</b>	1.30	<b>1.52</b>	1.66	<b>1.84</b>	1.99	<b>2.12</b>	2.25	<b>2.39</b>	2.55	<b>2.75</b>	3.05	<b>3.33</b>	3.91
5-7 years	<b>1.19</b>	1.42	<b>1.66</b>	1.81	<b>2.01</b>	2.16	<b>2.30</b>	2.44	<b>2.59</b>	2.76	<b>2.97</b>	3.29	<b>3.59</b>	4.2
7-9 y. boys	<b>1.25</b>	1.48	<b>1.73</b>	1.88	<b>2.07</b>	2.22	<b>2.36</b>	2.50	<b>2.65</b>	2.81	<b>3.02</b>	3.33	<b>3.61</b>	4.22
7-9 y. girls	<b>1.36</b>	1.61	<b>1.88</b>	2.04	<b>2.25</b>	2.42	<b>2.57</b>	2.72	<b>2.88</b>	3.06	<b>3.28</b>	3.62	<b>3.94</b>	4.58
9-11 y. boys	<b>1.47</b>	1.73	<b>1.99</b>	2.15	<b>2.36</b>	2.52	<b>2.66</b>	2.81	<b>2.96</b>	3.14	<b>3.35</b>	3.67	<b>3.97</b>	4.57
9-11 y. girls	<b>1.56</b>	1.90	<b>2.20</b>	2.38	<b>2.62</b>	2.80	<b>2.96</b>	3.13	<b>3.30</b>	3.50	<b>3.75</b>	4.11	<b>4.45</b>	5.16
11-13 y. boys	<b>1.58</b>	1.88	<b>2.19</b>	2.38	<b>2.63</b>	2.82	<b>3.00</b>	3.18	<b>3.37</b>	3.58	<b>3.84</b>	4.25	<b>4.62</b>	5.39
11-13 y. girls	<b>1.62</b>	1.90	<b>2.24</b>	2.46	<b>2.74</b>	2.97	<b>3.17</b>	3.38	<b>3.60</b>	3.85	<b>4.17</b>	4.65	<b>5.10</b>	6.02
13-15 y. boys	<b>1.62</b>	1.89	<b>2.24</b>	2.46	<b>2.76</b>	2.99	<b>3.20</b>	3.42	<b>3.65</b>	3.91	<b>4.24</b>	4.75	<b>5.22</b>	6.20
13-15 y. girls	<b>1.69</b>	2.03	<b>2.39</b>	2.61	<b>2.91</b>	3.14	<b>3.35</b>	3.56	<b>3.79</b>	4.04	<b>4.36</b>	4.85	<b>5.30</b>	6.24
15-17 y. boys	<b>1.70</b>	2.02	<b>2.36</b>	2.57	<b>2.84</b>	3.05	<b>3.25</b>	3.44	<b>3.65</b>	3.88	<b>4.17</b>	4.61	<b>5.01</b>	5.86
15-17 y. girls	<b>1.62</b>	1.93	<b>2.26</b>	2.46	<b>2.73</b>	2.93	<b>3.12</b>	3.31	<b>3.51</b>	3.74	<b>4.02</b>	4.45	<b>4.85</b>	5.67
17-20 y.	<b>1.58</b>	1.90	<b>2.24</b>	2.45	<b>2.72</b>	2.94	<b>3.13</b>	3.33	<b>3.54</b>	3.78	<b>4.07</b>	4.53	<b>4.95</b>	5.83
20-30 y.	<b>1.55</b>	1.86	<b>2.20</b>	2.41	<b>2.68</b>	2.90	<b>3.09</b>	3.29	<b>3.50</b>	3.74	<b>4.04</b>	4.50	<b>4.92</b>	5.80
30-40 y.	<b>1.44</b>	1.75	<b>2.08</b>	2.29	<b>2.56</b>	2.78	<b>2.98</b>	3.18	<b>3.39</b>	3.64	<b>3.95</b>	4.42	<b>4.86</b>	5.78
40-50 y.	<b>1.38</b>	1.68	<b>2.01</b>	2.21	<b>2.48</b>	2.69	<b>2.88</b>	3.08	<b>3.29</b>	3.53	<b>3.83</b>	4.29	<b>4.72</b>	5.63
50-60 y.	<b>1.34</b>	1.64	<b>1.96</b>	2.16	<b>2.42</b>	2.63	<b>2.83</b>	3.02	<b>3.23</b>	3.46	<b>3.76</b>	4.22	<b>4.65</b>	5.55
60-70 y.	<b>1.28</b>	1.58	<b>1.90</b>	2.10	<b>2.37</b>	2.58	<b>2.78</b>	2.98	<b>3.19</b>	3.44	<b>3.75</b>	4.23	<b>4.67</b>	5.62
70-80 y.	<b>1.20</b>	1.50	<b>1.81</b>	2.00	<b>2.27</b>	2.47	<b>2.67</b>	2.87	<b>3.08</b>	3.32	<b>3.62</b>	4.09	<b>4.52</b>	5.44
> 80 y.	<b>1.13</b>	1.43	<b>1.73</b>	1.92	<b>2.19</b>	2.39	<b>2.59</b>	2.79	<b>3.00</b>	3.23	<b>3.54</b>	4.00	<b>4.44</b>	5.36

Serum levels are given as mg/L  
y. = years

Determined with IGFBP-3 RIA (Blum et al. 1990)  
The values above 70 years are extrapolated.

**Serum conc. according to age**

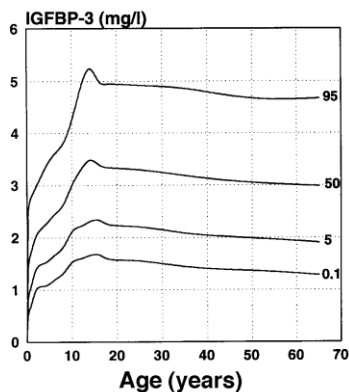


Fig. 5: Age-dependent normal values of IGFBP-3 (presented as 0.1., 5., 50., and 95. percentile)

**Children and adolescents**

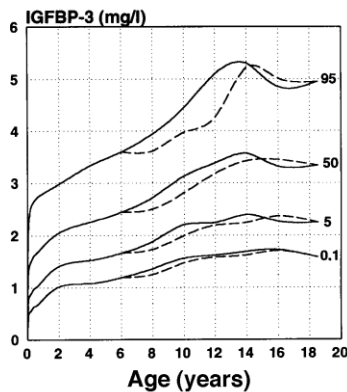


Fig. 6: Normal values of children and adolescents (girls — boys - - -)

## PERFORMANCE CHARACTERISTICS

### Sensitivity

Sensitivity was assessed by measuring the blank and calculating the theoretical concentration of the 2fold standard deviation of the blank. The analytical sensitivity of the E03A is 0.03 ng/mL.

According ICH Q2 R1 (CPMP/ICH/381/95) the limit of quantification (LoQ) is reflected by the recalculated IGFBP-3 concentration of the 10fold standard deviation of the blank, which therewith is 0.15 ng/mL.

### Specificity

The cross-reactivity of the antibodies used for Mediagnost IGFBP-3 ELISA to homologous proteins was evaluated by diluting IGFBP-1, -2,-4,-5 and -6 in assay buffer to a concentration of 200 ng/mL and subsequent measurement of IGFBP-3. The relative cross-reactivities were  $\leq 0.125\%$ .

### Reproducibility and Precision

#### Intra-Assay-Variation

One sample has been measured 10 times in the same assay. The results are shown in table 2. The measured coefficient of variation (CV) is on average 1.9%

**Tab. 2:** Intra-Assay-Variation. Three exemplary serum samples were diluted and measured 10 times within one assay.

	Sample 1	Sample 2	Sample 3
Mean [ng/mL]	3630	3789	3016
SD	70.83	83.75	46.71
%CV	1.95	2.21	1.55
n	10	10	10

#### Inter-assay-Variation

Serum samples were measured in independent assays on different days. On average the coefficient of variation was 5.7%. Results are shown in detail in table 3.

**Tab. 3:** Inter-Assay-Variation. Serum samples were diluted as recommended (1:505) and IGFBP-3 concentration was measured in different independent assays.

	Sample 1	Sample 2	Sample 3	Sample 4	Sample 5	Sample 6	Sample 7	Sample 8
Mean [ng/mL]	2886	3525	3229	3219	4025	3293	3889	4328
SD	193	178	140	237	171	177	199	322
%CV	6.68	5.05	4.34	7.36	4.25	5.38	5.12	7.44
n	4	10	9	7	10	10	7	10

### Linearity

Linearity was proven by dilution of three different serum samples with known IGFBP-3 concentration. The IGFBP-3 concentration of the diluted sample was measured and compared with the concentration expected. Results of linear regression analysis are shown in Figure 7. None of IGFBP-3 concentrations of the dilutions (1:125 to 1:2000) deviated more than 20% of the expected value ( $\leq -17\%$ ).

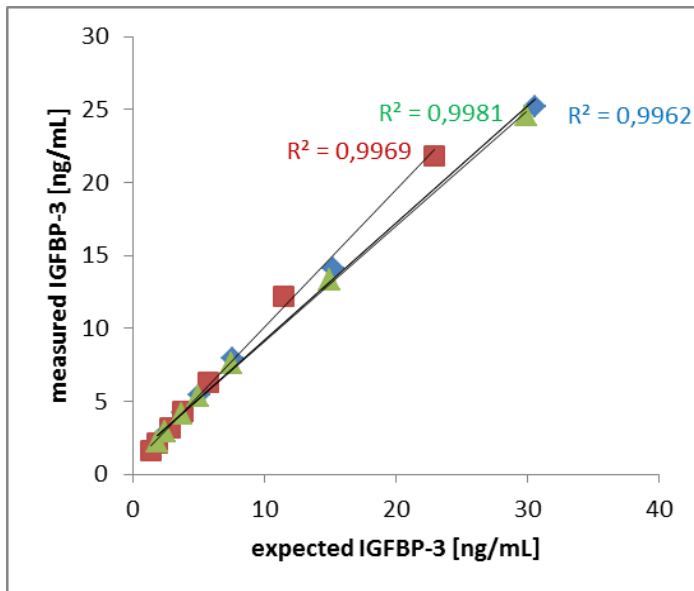


Fig. 7: Linearity. Shown are the measured concentrations in different dilutions of three serum samples.

### Recovery

Serum and plasma samples were enriched with recombinant IGFBP-3 and the recovery was calculated in comparison to buffer enriched with the same amount of IGFBP-3. The native samples used had an IGFBP-3 concentration of 2684 to 3667 ng/mL and the relative recovery was 109 – 118%. Results are shown in Table 4.

**Tab. 4: Recovery [%]** of recombinant IGFBP-3 in native serum/plasma samples in comparison to recombinant IGFBP-3 in buffer.

IGFBP-3		Sample [ng/mL]	Sample [ng/mL] enriched	Target value [ng/mL]	Recovery [%]
Sample 1	Plasma	3641	5107	4324	118
Sample 2	Plasma	3667	4778	4350	110
Sample 3	Serum	2869	3778	3552	106
Sample 4	Serum	2684	3677	3367	109

### Interference

Interference of physiological appearing substance with the IGFBP-3 measurement was investigated. Serum samples have been enriched with different concentrations of possibly interfering substances and the amount of IGFBP-3 was measured and compared with the IGFBP-3 concentration in the same sample without any enrichment. In Table 5 the relative results are shown. None of the tested substances interfered significantly with IGFBP-3 measurement.


**Tab. 5: Recovery [%]** in comparison to the native serum.

	Triglyceride 100 mg/mL	Bilirubin 100 µg/mL	Hemoglobin 5 mg/mL
Sample 1	89	93	81
Sample 2	87	91	106
Sample 3	88	96	93



### Comparison with other assays

The Mediagnost IGFBP-3 ELISA E03A was compared with the Mediagnost RIA test system (IGF-R10). In total 150 different samples with IGFBP-3 concentrations of 10 – 5118 ng/mL were used. The results are shown graphically in Figure 8. The relative deviation of Mediagnost RIA is on average 9.00% (0.18-28.29%).

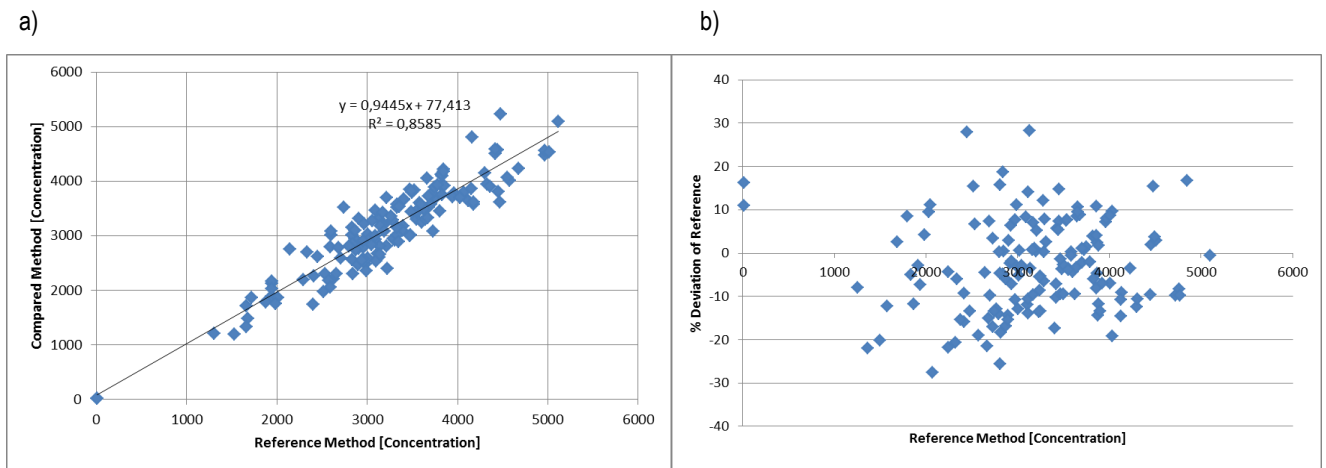

**Fig. 8:** Comparison of Mediagnost RIA to Mediagnost IGFBP-3 ELISA E03A with Fab Detection Antibody. IGFBP-3 concentration was measured in 150 samples with both assays. Here results are analysed by linear regression analysis (a) and Bland-Altman plot (b).

Further, data resulting from the external quality assessment provided by DGKL/ RfB (Germany) are shown (Table 6). Here the deviation of the concentrations measured by Mediagnost IGFBP-3 ELISA E03A from the method-specific and method-independent target value is shown. The deviation of the Method-specific target value is -17% and the deviation of the method-independent target value is -19% on average, which is within the acceptance criteria of the DGKL/RfB ( $\leq 30\%$ ).

**Tab. 6:** External Quality Assessment Scheme:

DGKL/RfB Germany retrospective analysis of 2013/2014 samples.

DGKL EQA		Mean	HP1/14	HP4/13	HP3/13	HP2/13	HP1/13
Measured Value [ng/mL]	Probe A	-	3608	3778	3163	3222	3144
Target Value [ng/mL]	Probe A	-	3377	3723	3532	3740	3889
Total Mean [ng/mL]	Probe A	-	3948	3899	3825	3826	3922
$\Delta$ A Targetvalue [%]	Probe A	-15.76	6.83	1.47	-10.46	-13.85	-19.16
$\Delta$ A Total Mean [%]	Probe A	-17.82	-8.62	-3.11	-17.32	-15.79	-19.84
DGKL EQA		Mean	HP1/14	HP4/13	HP3/13	HP2/13	HP1/13
Measured Value [ng/mL]	Probe B	-	3101	3588	3243	3098	3149
Target Value [ng/mL]	Probe B	-	3422	4008	3360	4170	3618
Total Mean [ng/mL]	Probe B	-	3941	3864	3846	3857	3873
$\Delta$ B Targetvalue [%]	Probe B	-18.84	-9.38	-10.47	-3.47	-25.71	-12.97
$\Delta$ B Total Mean [%]	Probe B	-19.19	-21.32	-7.14	-15.67	-19.68	-18.70

## LITREATURE

- 1) Ballard J, Baxter R, Binoux M, Clemmons D, Drop S, Hall K, Hintz R, Rechler M, Rutanen E, Schwander J (1989) On the nomenclature of the IGF binding proteins. *Acta Endocrinol (Copenh)* 121:751-752
- 2) Wilson EM, Oh Y, Rosenfeld RG (1997) Generation and characterization of an IGFBP-7 antibody: Identification of 31 kD IGFBP-7 in human biological fluids and Hs578T human breast cancer conditioned media. *J Clin Endocrinol Metab* Vol 82, 4:1301-1303
- 3) Baxter RC (1988) Characterization of the acid-labile subunit of the growth hormone-dependent insulin-like growth factor binding protein complex. *J Clin Endocrinol Metab* 67:265-272
- 4) Baxter RC, Martin JL (1989) Structure of the Mr 140,000 growth hormone dependent insulin-like growth factor binding protein complex: determination by reconstitution and affinity-labeling. *Proc Natl Acad Sci USA* 86:6898-6902
- 5) Holman SR, Baxter RC (1996) Insulin-like growth factor-binding protein-3: factors affecting binary and ternary complex formation. *Growth Regulation* 6: 42-47.
- 6) Baxter RC, Martin J (1986): Radioimmunoassay of growth hormone-dependent insulin-like growth factor binding protein in human plasma. *J Clin Invest* 78:1504-1512
- 7) Blum WF, Ranke MB, Kietzmann K, Gauggel E, Zeissel HJ, Bierich JR (1990) A specific radioimmunoassay for the growth hormone (GH)-dependent somatomedin-binding protein: its use for diagnosis of GH deficiency. *J Clin Endocrinol Metab* 70:1292-1298
- 8) Blum WF, Ranke MB (1990) Use of insulin-like growth factor binding protein 3 for the evaluation of growth disorders. *Horm Res* 34 (Suppl):31-37
- 9) Blum WF (1993) Insulin-like growth factor-binding protein 3: Entwicklung eines Radioimmunoassays und Untersuchungen zur klinischen Bedeutung. *Habilitationsschrift, Tübingen.*
- 10) Lee PDK, Hintz RL, Sperry JB, Baxter RC, Powell DR (1989) IGF-binding proteins in growth-retarded children with chronic renal failure. *Pediatr Res* 26:308-315
- 11) Blum WF, Ranke MB, Kietzmann K, Tönshoff B, Mehls O (1989) Excess of IGF-binding proteins in chronic renal failure: evidence for relative GH resistance and inhibition of somatomedin activity. In: Drop SLS, Hintz RL (eds) *Insulin-like Growth Factor Binding Proteins*. Excerpta Medica, Amsterdam, pp 93-101
- 12) Baxter RC, Cowell CT (1987) Diurnal rhythm of growth hormone-independent binding protein for insulin-like growth factors in human plasma. *J Clin Endocrinol Metab* 65:432-440
- 13) Jorgensen JOL, Blum WF, Moller N, Ranke MB, Christiansen JS (1990) Circadian patterns of serum insulin-like growth factor (IGF)-II and IGF-binding protein 3 in growth hormone deficient patients and age- and sex-matched normal subjects. *Acta Endocrinol (Copenh.)* 123:257-262
- 14) Blum WF, Albertsson-Wikland K, Rosberg S, Jorgensen JOL, Ranke MB (1990) Insulin-like growth factor binding protein 3 (IGFBP-3) reflects spontaneous growth hormone (GH) secretion. *Horm Res* 33 (Suppl 3): 3

(Abstract)


- 15) Blum WF, Ranke MB (1990) Insulin-like growth factor-binding proteins (IGFBPs) with special reference to IGFBP-3. *Acta Paediatr Scand (Suppl)* 367:55-62
- 16) Giudice LC, Farrell EM, Pham H, Lamson G, Rosenfeld RG (1990) Insulin-like growth factor binding proteins in maternal serum throughout gestation and in the puerperium: effects of a pregnancy-associated serum protease activity. *J Clin Endocrinol Metab* 71:806-816
- 17) Hossenlopp P, Segovia B, Lassarre C, Roghani M, Bredon M, Binoux M (1990) Evidence of enzymatic degradation of insulin-like growth factor-binding proteins in the 150k complex during pregnancy. *J Clin Endocrinol Metab* 71:797-805
- 18) Ranke MB, Schweizer R, Elmlinger MW, Weber K, Binder G, Schwarze CP, Wollmann HA (2000) Significance of Basal IGF-I, IGFBP-3 and IGFBP-2 Measurements in the diagnostics of short stature in children. *Horm Res* 2000;54:60-68
- 19) Ranke MB, Schweizer R, Elmlinger MW, Weber K, Binder G, Schwarze CP, Wollmann HA (2001) Relevance of IGF-I, IGFBP-3, and IGFBP-2 Measurements during GH treatment of GH-deficient and non-GH-deficient children and adolescents. *Horm Res* 2001;55:115-124
- 20) Langkamp M, Weber K., Kirschner M., Pridzun L., Ranke M.B. Validation of Functional insulin-Like Growth Factor Binding Protein-3 measurement by a Ligand Immunoassay. *Clin Lab.* 11+12/2010, 56; 535-542



A-E	STD	Rec in 1 mL	BUF PP	-
KS1	Control	Rec in 250 µL	BUF PP	1:505 DILU BUF PP
KS2	Control	Rec in 250 µL	BUF PP	1:505 DILU BUF PP
WP	WASHBUF 20x	-		1:20 DILU A. dest.
-	SPE			1:505 DILU BUF PP
-	°C 20-25 °C			
50 µL	BUF VP			A1 - End
50 µL	BUF PP			A1/A2
50 µL	STD A	(0.4 ng/mL)		B1/B2
50 µL	STD B	(2 ng/mL)		C1/C2
50 µL	STD C	(6 ng/mL)		D1/D2
50 µL	STD D	(15 ng/mL)		E1/E2
50 µL	STD E	(30 ng/mL)		F1/F2
50 µL	CONTROL KS1 1:505 DILU BUF PP			G1/G2
50 µL	CONTROL KS2 1:505 DILU BUF PP			H1/H2
50 µL	SPE	1:505 DILU BUF PP		
TAPE				
⌚ 1 h °C 20-25 350 rpm <span style="border: 1px solid black; padding: 2px;">↔</span>				
5x 300 µL	5x WASHBUF WP			
100 µL	Ab CONJ AK			
TAPE				
⌚ 1 h °C 20-25 350 rpm <span style="border: 1px solid black; padding: 2px;">↔</span>				
5x 300 µL	5x WASHBUF WP			
100 µL	SUBST TMB S			
⌚ 0.5 h °C 20-25				
H <sub>2</sub> SO <sub>4</sub> SL				

**MEASURE**



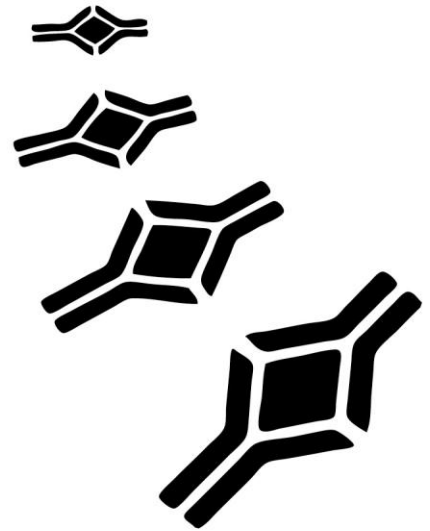

*Distributed by:*

**BioVendor – Laboratorní medicína a.s.**

Karasek 1767/1, 621 00 Brno, Czech Republic

Phone: +420-549-124-185, Fax: +420-549-211-460

E-mail: [info@biovendor.com](mailto:info@biovendor.com), [sales@biovendor.com](mailto:sales@biovendor.com)

Web: [www.biovendor.com](http://www.biovendor.com)

*Manufactured by:*

**Mediagnost®**

Aspenhastr. 25, D-71770 Reutlingen, Germany

E-mail: [contact@mediagnost.de](mailto:contact@mediagnost.de)

Web: [www.mediagnost.de](http://www.mediagnost.de)



There are BioVendor branches and distributors near you. To find the office closest to you, visit [www.biovendor.com/contact](http://www.biovendor.com/contact)