

BioVendor

Research
and Diagnostic Products



HUMAN SYNDECAN-1 (CD138) ELISA

Product Data Sheet

Cat. No.: RGP009R

For Research Use Only

CONTENTS

| | | |
|-----|---|----|
| 1. | INTENDED USE | 3 |
| 2. | INTRODUCTION | 3 |
| 3. | PRINCIPLE OF THE METHOD | 3 |
| 4. | REAGENTS PROVIDED AND RECONSTITUTION | 4 |
| 5. | MATERIAL REQUIRED BUT NOT PROVIDED | 5 |
| 6. | STORAGE INSTRUCTIONS | 5 |
| 7. | SPECIMEN COLLECTION, PROCESSING & STORAGE | 5 |
| 8. | SAFETY & PRECAUTIONS FOR USE | 6 |
| 9. | ASSAY PREPARATION | 7 |
| 10. | METHOD | 10 |
| 11. | DATA ANALYSIS | 11 |
| 12. | ASSAY LIMITATIONS | 12 |
| 13. | PERFORMANCE CHARACTERISTICS | 12 |
| 14. | REFERENCES | 14 |
| 15. | HUMAN CD138 ELISA REFERENCES | 15 |
| 16. | ASSAY SUMMARY | 16 |

**»» This kit is manufactured by:
BioVendor – Laboratorní medicína a.s.**

»» Use only the current version of Product Data Sheet enclosed with the kit!

1. INTENDED USE

The Syndecan-1 (CD138) ELISA kit is a solid phase sandwich ELISA for research use only qualitative and quantitative determination of sCD138 in supernatants, buffered solutions or serum and plasma samples. This assay will recognise both natural and recombinant human sCD138.

This kit has been configured for research only. Not suitable for use in therapeutic procedures.

2. INTRODUCTION

Syndecans are a transmembrane protein family within the heparin sulphate proteoglycan group that interact with many different molecules of the immune system through their heparin sulphate chains. The mammalian syndecan family consists of 4 proteins; syndecan 1 to 4 each encoded by very distinct genes. In adult tissues syndecan 1 (CD138) is predominantly expressed by epithelial cells and plasma cells (both normal and malignant) and currently considered the most reliable surface marker for plasma cells. In addition CD138 is also expressed on pre and immature B cells however this is regulated by IL-6 and LPS stimulation. Syndecan 1 has previously been shown to participate in cell to cell interactions, organ development, vessel formation and tissue regeneration following injury.

CD138 is regularly cleaved from the membrane and as a consequence high levels of soluble CD138 are found in the blood, which can be easily detected using a CD138 specific ELISA.

Via its heparin sulphate chains CD138 binds to and modulates the activity of a wide range of molecules involve in inflammation including chemokines, growth factors, selectins and other adhesion molecules. CD138 can also act as a receptor for collagen, fibronectin, thrombospondin and tenascin therefore involved in cell matrix adhesion. CD138 has been shown to mediate the binding of myeloma cells to type I collagen, and inhibits tumour cell invasion into collagen gels.

As CD138 has been shown to have important effects on tumour cell growth, survival, adhesion and invasion syndecan-1 may be an important regulator in cancer biology.

3. PRINCIPLE OF THE METHOD

A capture Antibody highly specific for CD138 has been coated to the wells of the microtitre strip plate provided during manufacture. Binding of CD138 samples and known standards to the capture antibodies and subsequent binding of the biotinylated anti-CD138 secondary antibody to the analyte is completed during the same incubation period. Any excess unbound analyte and secondary antibody is removed. The HRP conjugate solution is then added to every well including the zero wells, following incubation excess conjugate is removed by careful washing.

A chromogen substrate is added to the wells resulting in the progressive development of a blue coloured complex with the conjugate.

The colour development is then stopped by the addition of acid turning the resultant final product yellow. The intensity of the produced coloured complex is directly proportional to the concentration of CD138 present in the samples and standards. The absorbance of the colour complex is then measured and the generated OD values for each standard are plotted against expected concentration forming a standard curve. This standard curve can then be used to accurately determine the concentration of CD138 in any sample tested.

4. REAGENTS PROVIDED AND RECONSTITUTION

| REAGENTS (Store at 2-8°C) | Quantity | State |
|--|-----------------|---|
| Antibody Coated Microtiter Strips | 96 wells | Ready to use (Pre-coated) |
| Plastic plate covers | 2 vials | n/a |
| Standard: 256 ng/ml | 2 vials | Reconstitute as directed in the Quality Control Sheet (see reagent preparation) |
| Standard Diluent (Buffer) | 1 vial (25 ml) | 10x Concentrate, dilute in distilled water (see reagent preparation) |
| Control | 2 vials | Reconstitute as directed Quality Control Sheet (see reagent preparation) |
| Biotinylated anti-CD138 | 1 vial (0.4 ml) | Dilute in biotinylated antibody diluent (see reagent preparation) |
| Biotinylated Antibody diluent | 1 vial (7 ml) | Ready to use |
| Streptavidin-HRP | 2 vial (5 µl) | Add 0.5 ml of HRP diluent prior to use (see reagent preparation) |
| HRP Diluent | 1 vial (23 ml) | Ready to use |
| Wash Buffer | 1 vial (10 ml) | 200x Concentrate dilute in distilled water (see reagent preparation) |
| TMB Substrate: | 1 vial (11 ml) | Ready to use |
| H ₂ SO ₄ : Stop Reagent | 1 vial (11 ml) | Ready to use |

5. MATERIAL REQUIRED BUT NOT PROVIDED

- Microtitre plate reader fitted with appropriate filters (450 nm required with optional 620 nm reference filter)
- Microplate washer or wash bottle
- 10, 50, 100, 200 and 1,000 µl adjustable single channel micropipettes with disposable tips
- 50-300 µl multi-channel micropipette with disposable tips
- Multichannel micropipette reagent reservoirs
- Distilled water
- Vortex mixer
- Miscellaneous laboratory plastic and/or glass, if possible sterile

6. STORAGE INSTRUCTIONS

Store kit reagents between 2 and 8°C. Immediately after use remaining reagents should be returned to cold storage (2-8°C). Expiry of the kit and reagents is stated on box front labels. The expiry of the kit components can only be guaranteed if the components are stored properly, and if, in case of repeated use of one component, the reagent is not contaminated by the first handling.

7. SPECIMEN COLLECTION, PROCESSING & STORAGE

Cell culture supernatants, human serum, plasma or other biological samples will be suitable for use in the assay. Remove serum from the clot or red cells, respectively, as soon as possible after clotting and separation.

Cell culture supernatants: Remove particulates and aggregates by spinning at approximately 1000 x g for 10 min.

Serum: Use pyrogen/endotoxin free collecting tubes. Serum should be removed rapidly and carefully from the red cells after clotting. Following clotting, centrifuge at approximately 1000 x g for 10 min and remove serum.

Plasma: EDTA, citrate and heparin plasma can be assayed. Spin samples at 1000 x g for 30 min to remove particulates. Harvest plasma.

Storage: If not analyzed shortly after collection, samples should be aliquoted (250-500 µl) to avoid repeated freeze-thaw cycles and stored frozen at -70°C. Avoid multiple freeze-thaw cycles of frozen specimens.

Recommendation: Do not thaw by heating at 37°C or 56°C. Thaw at room temperature and make sure that sample is completely thawed and homogeneous before use. When possible avoid use of badly haemolysed or lipemic sera. If large amounts of particles are present these should be removed prior to use by centrifugation or filtration.

8. SAFETY & PRECAUTIONS FOR USE

- Handling of reagents, serum or plasma specimens should be in accordance with local safety procedures , e.g.CDC/NIH Health manual : " Biosafety in Microbiological and Biomedical Laboratories" 1984
- Laboratory gloves should be worn at all times
- Avoid any skin contact with H₂SO₄ and TMB. In case of contact, wash thoroughly with water
- Do not eat, drink, smoke or apply cosmetics where kit reagents are used
- Do not pipette by mouth
- When not in use, kit components should be stored refrigerated or frozen as indicated on vials or bottles labels
- All reagents should be warmed to room temperature before use. Lyophilized standards should be discarded after use
- Once the desired number of strips has been removed, immediately reseal the bag to protect the remaining strips from deterioration
- Cover or cap all reagents when not in use
- Do not mix or interchange reagents between different lots
- Do not use reagents beyond the expiration date of the kit
- Use a clean disposable plastic pipette tip for each reagent, standard, or specimen addition in order to avoid cross contamination, for the dispensing of H₂SO₄ and substrate solution, avoid pipettes with metal parts
- Use a clean plastic container to prepare the washing solution
- Thoroughly mix the reagents and samples before use by agitation or swirling
- All residual washing liquid must be drained from the wells by efficient aspiration or by decantation followed by tapping the plate forcefully on absorbent paper. Never insert absorbent paper directly into the wells
- The TMB solution is light sensitive. Avoid prolonged exposure to light. Also, avoid contact of the TMB solution with metal to prevent colour development. Warning TMB is toxic avoid direct contact with hands. Dispose off properly
- If a dark blue colour develops within a few minutes after preparation, this indicates that the TMB solution has been contaminated and must be discarded. Read absorbance's within 1 hour after completion of the assay
- When pipetting reagents, maintain a consistent order of addition from well-to-well. This will ensure equal incubation times for all wells
- Follow incubation times described in the assay procedure
- Dispense the TMB solution within 15 min of the washing of the microtitre plate

9.2. Preparation of Wash Buffer

Dilute the (200x) wash buffer concentrate 200 fold with distilled water to give a 1x working solution. Pour entire contents (10 ml) of the Washing Buffer Concentrate into a clean 2,000 ml graduated cylinder. Bring final volume to 2,000 ml with glass-distilled or deionized water. Mix gently to avoid foaming. Transfer to a clean wash bottle and store at 2°-25°C.

9.3. Preparation of Standard Diluent Buffer

Add the contents of the vial (10x concentrate) to 225ml of distilled water before use. This Solution can be stored at 2-8°C for up to 1 week.

9.4. Preparation of Standard

Standard vials must be reconstituted with the volume of standard diluent shown Quality Control Sheet immediately prior to use. This reconstitution gives a stock solution of 256 ng/ml of CD138. Mix the reconstituted standard gently by inversion only. Serial dilutions of the standard are made directly in the assay plate to provide the concentration range from 256 to 8ng/ml. A fresh standard curve should be produced for each new assay.

- Immediately after reconstitution add 200 µl of the reconstituted standard to well's A1 and A2, which provides the highest concentration standard at 256 ng/ml
- Add 100 µl of appropriate standard diluent to the remaining standard wells B1 and B2 to F1 and F2.
- Transfer 100 µl from wells A1 and A2 to B1 and B2. Mix the well contents by repeated aspirations and ejections taking care not to scratch the inner surface of the wells
- Continue this 1:1 dilution using 100 µl from wells B1 and B2 through to wells F1 and F2 providing a serial diluted standard curve ranging from 256 ng/ml to 8 ng/ml
- Discard 100 µl from the final wells of the standard curve (F1 and F2)

Alternatively these dilutions can be performed in separate clean tubes and immediately transferred directly into the relevant wells.

9.5. Preparation of Controls

The supplied Controls must be reconstituted with the volume of Standard Diluent indicated Quality Control Sheet. Reconstitution of the freeze-dried material with the indicated volume, will give a solution at the concentration stated on the vial. Do not store after use.

9.6. Preparation of Biotinylated anti-CD138

It is recommended this reagent is prepared immediately before use. Dilute the biotinylated anti-IL-8 with the biotinylated antibody diluent in an appropriate clean glass vial using volumes appropriate to the number of required wells. Please see example volumes below:

| Number of Wells used | Biotinylated Antibody (μ l) | Biotinylated Antibody Diluent (μ l) |
|----------------------|----------------------------------|--|
| 16 | 40 | 1060 |
| 24 | 60 | 1590 |
| 32 | 80 | 2120 |
| 48 | 120 | 3180 |
| 96 | 240 | 6360 |

9.7. Preparation of Streptavidin-HRP

It is recommended to centrifuge vial for a few seconds in a microcentrifuge to collect all the volume at the bottom.

Dilute the 5 μ l vial with 0.5 ml of HRP diluent immediately before use. Do-not keep this diluted vial for future experiments. Further dilute the HRP solution to volumes appropriate for the number of required wells in a clean glass vial. Please see example volumes below:

| Number of Wells | Streptavidin-HRP(μ l) | Strep-HRP Diluent (ml) |
|-----------------|----------------------------|------------------------|
| 16 | 30 | 2 |
| 24 | 45 | 3 |
| 32 | 60 | 4 |
| 48 | 75 | 5 |
| 96 | 150 | 10 |

10. METHOD

We strongly recommend that every vial is mixed thoroughly without foaming prior to use.

Prepare all reagents as shown in section 8.

Note: final preparation of Biotinylated Secondary Antibody (section 8.6) and Streptavidin-HRP (section 8.7) should occur immediately before use.

| Assay Step | Details |
|---|--|
| 1. Addition | Prepare Standard curve as shown in section 8.4 above |
| 2. Addition | Add 100 µl of each, Sample, Standard, Control and zero (Standard diluent) in duplicate to appropriate number of wells |
| 3. Addition | Add 50 µl of diluted biotinylated anti-CD138 to all wells |
| 4. Incubation | Cover with a plastic plate cover and incubate at room temperature (18 to 25°C) for 1 hour(s) |
| 5. Wash | Remove the cover and wash the plate as follows: a) Aspirate the liquid from each well b) Dispense 0.3 ml of 1x washing solution into each well c) Aspirate the contents of each well d) Repeat step b and c another two times |
| 6. Addition | Add 100 µl of Streptavidin-HRP solution into all wells |
| 7. Incubation | Cover with a plastic plate cover and incubate at room temperature (18 to 25°C) for 30 min |
| 8. Wash | Repeat wash step 5. |
| 9. Addition | Add 100 µl of ready-to-use TMB Substrate Solution into all wells |
| 10. Incubation | Incubate in the dark for 12-15 minutes* at room temperature. Avoid direct exposure to light by wrapping the plate in aluminium foil. |
| 11. Addition | Add 100 µl of H₂SO₄:Stop Reagent into all wells |
| Read the absorbance value of each well (immediately after step 11.) on a spectrophotometer using 450 nm as the primary wavelength and optionally 620 nm as the reference wave length (610 nm to 650 nm is acceptable). | |


**Incubation time of the substrate solution is usually determined by the ELISA reader performance. Many ELISA readers only record absorbance up to 2.0 O.D. Therefore the colour development within individual microwells must be observed by the analyst, and the substrate reaction stopped before positive wells are no longer within recordable range*

11. DATA ANALYSIS

Calculate the average absorbance values for each set of duplicate standards, controls and samples. Ideally duplicates should be within 20% of the mean.

Generate a linear standard curve by plotting the average absorbance of each standard on the vertical axis versus the corresponding CD138 standard concentration on the horizontal axis.

The amount of CD138 in each sample is determined by extrapolating OD values against CD138 standard concentrations using the standard curve.

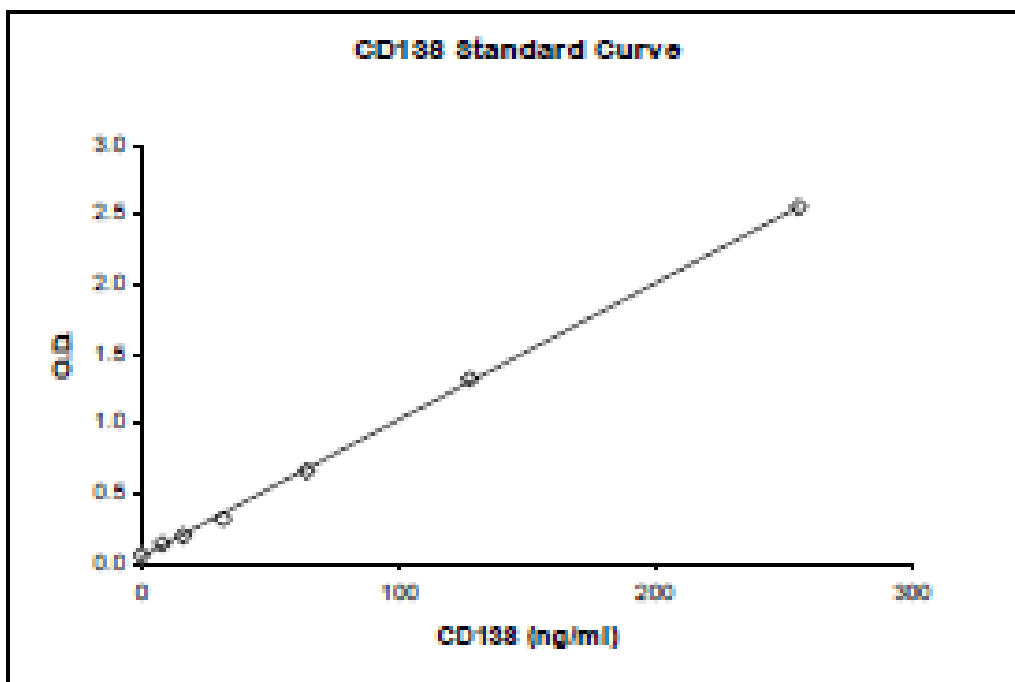

Example sCD138 Standard curve

| Standard | CD138 Conc | OD (450 nm) mean | CV (%) |
|----------|------------|------------------|--------|
| 1 | 256 | 2,554 | 7,4 |
| 2 | 128 | 1,317 | 10,8 |
| 3 | 64 | 0,667 | 2,0 |
| 4 | 32 | 0,320 | 8,8 |
| 5 | 16 | 0,199 | 1,4 |
| 6 | 8 | 0,132 | 9,1 |
| zero | 0 | 0,053 | 24,0 |

Note: curve shown above should not be used to determine results. Every laboratory must produce a standard curve for each set of microwell strips assayed.

12. ASSAY LIMITATIONS

Do not extrapolate the standard curve beyond the maximum standard curve point. The dose-response is non-linear in this region and good accuracy is difficult to obtain. Concentrated samples above the maximum standard concentration must be diluted with Standard diluent or with your own sample buffer to produce an OD value within the range of the standard curve. Following analysis of such samples always multiply results by the appropriate dilution factor to produce actual final concentration.

The influence of various drugs on end results has not been investigated. Bacterial or fungal contamination and laboratory cross-contamination may also cause irregular results.

Improper or insufficient washing at any stage of the procedure will result in either false positive or false negative results. Completely empty wells before dispensing fresh Washing Buffer, fill with Washing Buffer as indicated for each wash cycle and do not allow wells to sit uncovered or dry for extended periods. Disposable pipette tips, flasks or glassware are preferred, reusable glassware must be washed and thoroughly rinsed of all detergents before use.

As with most biological assays conditions may vary from assay to assay therefore **a fresh standard curve must be prepared and run for every assay.**

13. PERFORMANCE CHARACTERISTICS

13.1 Sensitivity

The sensitivity or minimum detectable dose of CD138 using this CD138 ELISA kit was found to be **4.94 ng/ml**. This was determined by adding 2 standard deviations to the mean OD obtained when the zero standard was assayed in 6 independent experiments.

13.2 Specificity

The assay recognizes both natural and recombinant human CD138. To define the specificity of this ELISA several proteins were tested for cross reactivity.

There was no cross reactivity observed for any protein tested (IL-1b, IL-2 IL-4, IFN γ , IL-6, IL-6R, TRAIL, IL-7, IL-12 and IL-21).

13.3 Precision

13.3.1 Intra-assay

Reproducibility within the assay will be evaluated in three independent experiments. Each assay will be carried out with 6 replicates (3 duplicates) in 2 human pooled serum, 2 in RPMI and 2 in standard diluent with samples containing different concentrations of CD138. 2 standard curves were run on each plate **The overall intra-assay coefficient of variation has been calculated to be 6.2%.**

| Session | Sample | Mean CD138 ng/ml | SD | CV |
|-----------|----------|------------------|-------|------|
| Session 1 | Sample 1 | 194,01 | 17,20 | 8,9 |
| | Sample 2 | 86,13 | 7,09 | 8,2 |
| | Sample 3 | 195,00 | 16,10 | 8,3 |
| | Sample 4 | 86,75 | 7,04 | 8,1 |
| | Sample 5 | 294,13 | 31,93 | 10,9 |
| | Sample 6 | 174,58 | 15,30 | 8,8 |
| Session 2 | Sample 1 | 171,65 | 3,94 | 2,3 |
| | Sample 2 | 79,97 | 5,85 | 7,3 |
| | Sample 3 | 173,60 | 5,80 | 3,3 |
| | Sample 4 | 76,61 | 2,42 | 3,2 |
| | Sample 5 | 242,90 | 15,80 | 6,5 |
| | Sample 6 | 169,50 | 7,72 | 4,6 |
| Session 3 | Sample 1 | 183,07 | 11,48 | 6,3 |
| | Sample 2 | 90,91 | 4,18 | 4,6 |
| | Sample 3 | 191,82 | 10,77 | 5,6 |
| | Sample 4 | 93,35 | 3,92 | 4,2 |
| | Sample 5 | 264,00 | 14,66 | 5,6 |
| | Sample 6 | 158,20 | 8,64 | 5,5 |

13.3.2 Inter-assay

Assay to assay reproducibility within one laboratory will be evaluated in three independent experiments by two technicians. Each assay will be carried out with 6 replicates (3 duplicates) in 2 human pooled serum, 2 in RPMI and 2 in standard diluent with samples containing different concentrations of CD138. 2 standard curves were run on each plate. **The calculated overall coefficient of variation was 10.2%.**

| | Sample 1 | Sample 2 | Sample 3 | Sample 4 | Sample 5 | Sample 6 |
|------------------|----------|----------|----------|----------|----------|----------|
| Mean CD138 ng/ml | 197 | 88 | 199 | 88 | 274 | 162 |
| SD | 21 | 8 | 19 | 9 | 27 | 19 |
| CV | 10,5 | 9,5 | 9,4 | 10,0 | 9,9 | 12,0 |

13.4 Dilution Linearity

In two independent experiments two spiked human serum samples with different levels of CD138 were analysed at different serial two fold dilutions (1:2 To 1:8) with two replicates each. Recoveries ranged from 59 to 122% with an overall **mean recovery of 85%.**

13.5 Spiking Recovery

The spiking recovery was evaluated by spiking 3 concentrations of CD138 in human serum and culture medium in 3 separate experiments. Recoveries ranged from 87 to 113% with an overall **mean recovery of 101%**

13.6 Stability

13.6.1 Storage Stability

Aliquots of spiked serum and spiked medium were stored at -20°C , 4°C , room temperature (RT) and at 37°C and the CD138 level determined after 24h. There was no significant loss of CD138 reactivity during storage at 4°C , RT and 37°C .

13.6.2 Freeze-thaw Stability

Aliquots of spiked serum and spiked medium were stored frozen at -20°C and thawed up to 5 times and the CD138 level was determined. There was no significant loss of CD138 reactivity after 5 cycles of freezing and thawing.

13.7 Expected serum values

A panel of 40 human sera and 40 Plasma samples were tested for CD138. See results below

| Sample Matrix | Number of samples evaluated | Range (ng/ml) | Mean (ng/ml) | Standard deviation (ng/ml) |
|---------------|-----------------------------|---------------|--------------|----------------------------|
| Serum | 40 | 16.17-205.16 | 48.15 | 36.5 |
| Plasma | 40 | 15.7-68.9 | 31.62 | 15.3 |

14. REFERENCES


1. Bartlett A et.al. Molecular and cellular mechanisms of syndecans in tissue injury and inflammation. *Mol. Cells*, Vol 24, No. 2. pp. 153-166. 2007
2. Gotte et.al. Syndecan-1 as a regulator of chemokine function. *The Scientific world*, 3, pp. 1327-1331. 2003
3. Gotte et.al. Syndecans in Inflammation. *FASEB*, 17, pp. 575-591. 2003
4. Masouleh et al. Role of the Heparin Sulphate Proteoglycan Syndecan-1 (CD138) in Delayed type Hypersensitivity. *Journal of immunology*, 182, pp. 4985-4993. 2009
5. Wanping Sun et.al. A Novel Anti-Human Syndecan-1(CD138) Monoclonal Antibody 4B3: Characterization and Application. *Cellular & Molecular Immunology*, 209, Volume 4, 2007.
6. Wijdenes J., Clement C., Klein B, Dore J-M. (1997). CD138 (syndecan-1) Workshop Panel report.
7. Wijdenes J., Dore JM., Clement C., Vermot-Desroches C.(2002) CD138 *J.Biol.Regul.Homeost. Agents* 16: 152-155.

15. HUMAN CD138 ELISA REFERENCES


1. Annecke, T. et al., *Br. J. Anaesth.*,2010;104(4): 414-421
2. Bruegger D. et al., *Am J Physiol Heart Circ Physiol*, 2005; 289(5):H1993-9
3. Bruegger, D. et al., *J. Thorac. Cardiovasc. Surg.*,2009;138(6): 1445-1447
4. Celie, J. W. A. M. et al., *Am J Physiol Renal Physiol.*,2008; 294(1): F253-263.
5. Chappell, D. et al.,*Cardiovasc. Res.*,2009;83(2):388-396
6. Iwata, H. et al., *Haematologica*,2004; 89(3): 368-370.
7. Janosi, J. et al., *Haematologica*,2004; 89(3): 370-371.
8. Joensuu H. et al., *Cancer Res.*, 2002; 62 : 5833 - 5842
9. Kliment,C.R. et al.,*J Biol. Chem.*, 2009 ; 284(6):3537-3545
10. Kyrtsolis M-C. et al., *Blood*, 2004; 104(11): 4882
11. Kyrtsolis, M.-C. et al.,*Blood (ASH Annual Meeting Abstracts)*,2005;106(11): 3404.
12. Mahtouk, K. et al.,*Blood*,2007;109: 4914 - 4923
13. Meuwese, M. C. et al., *J. Lipid Res.*,2008; P800025-JLR200.
14. Molica, S. et al.,*Leuk Lymphoma*, 2006; 47(6): 1034-40.
15. Rehm, M. et al., *Circulation*,2007; 116(17): 1896-1906.
16. Schaar, C. G. et al., *Haematologica*,2005; 90(10): 1437-1438.
17. Seidel C. et al., *Blood*, 2000; 95 : 388 - 392
18. Theocharis, A. D. et al.,*J Biol Chem.*,2006; 281(46): 35116-28.
19. Thiara, A. S. et al, *Perfusion*,2010; 25(1): 9-16


16. ASSAY SUMMARY

Total procedure length 1 h 45 mn

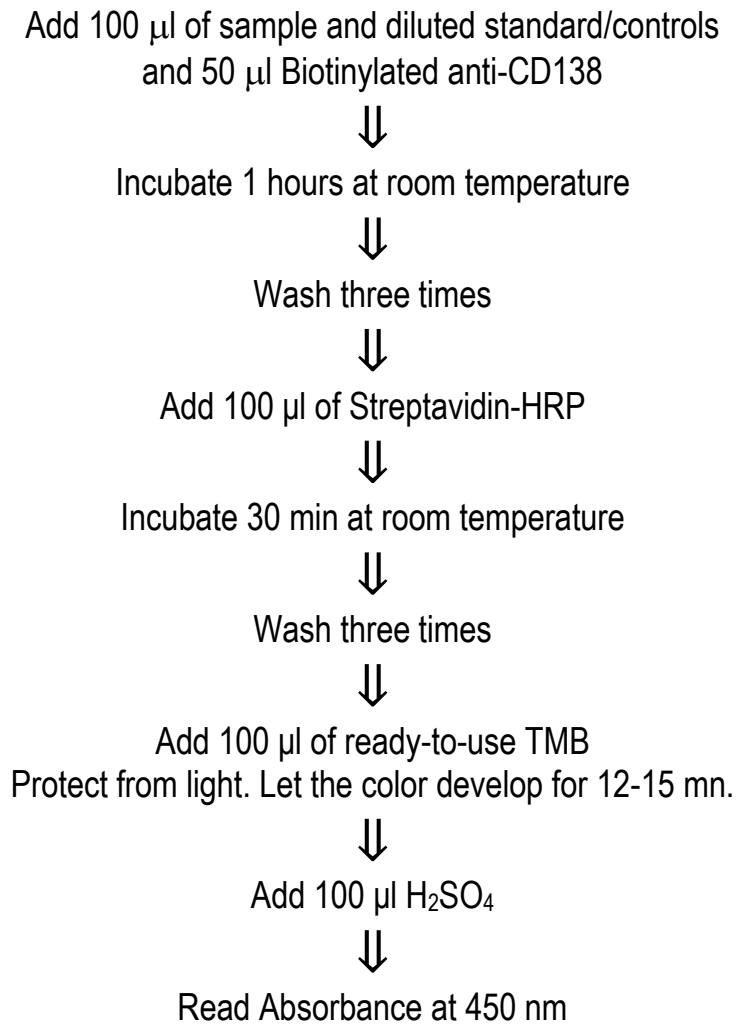

NOTES



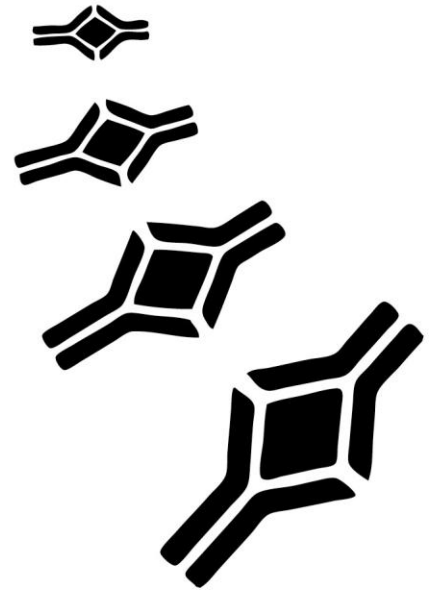

BioVendor – Laboratorní medicína, a.s.

Karasek 1767/1, 621 00 Brno, Czech Republic

Phone: +420-549-124-185, Fax: +420-549-211-460

E-mail: info@biovendor.com, sales@biovendor.com

Web: www.biovendor.com

There are BioVendor branches and distributors near you.

To find the office closest to you, visit www.biovendor.com/contact

